

ABSolu™

IMAGING
EXCELLENCE



A/B/S/UBM Ultrasound Platform



ABSolu™

■ NEW ANNULAR IMAGING

Quantel Medical has made a decisive leap forward with a new 5 ring annular technology on a 20 MHz probe.

The principle is to **emit alternating ultrasounds** by **5 concentric transducers** located in a single probe.

This technology:

- increases **depth of field** by 70%,
- increases **lateral resolution** by 27%,
- **maintains high axial resolution.**

The images thus obtained are spectacular as the **entire eye is now visible** with an exceptional level of **detail**.

Posterior lens capsule*

Detached retina with haemorrhaging*


Vitreo-retinal traction*

Weiss ring*

* © Peter Good, MD, Birmingham and Midland Eye Center (Birmingham, UK).

■ A SINGLE MULTIFUNCTION PROBE

The annular technology almost **doubles the depth of field** : the new 20 MHz annular probe increases the depth of field by 70% and makes it possible to **simultaneously examine** pathologies of the **vitreous**, the **retina** and the **orbit** without compromising on image quality.

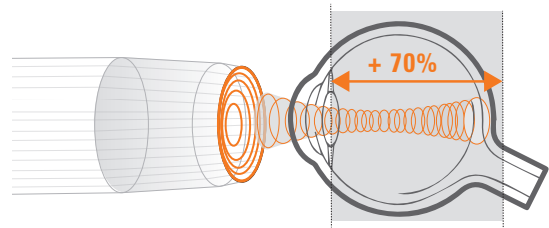

A/B/S/UBM Ultrasound Platform

REDESIGNED USER INTERFACE

The new ABSolu's user interface is intuitive and easy to use. It shortens the learning curve and makes it more fun to use.

- Broad palette of measuring tools.
- Display in B+B mode for easy comparisons of examinations.
- Fully configurable patient report generator.

ABSolu is also EMR compatible and connects to most data transfer and storage applications.

INTEGRATED MOTION SENSOR

The B15, B20 and UBM probes are equipped with a position sensor that provides real-time essential informations such as:

- the position of the probe on the eye,
- the direction of the ultrasound beam.

This helps the operator to identify the area of examination more rapidly.

THIS TECHNOLOGY IS PATENTED AND EXCLUSIVE TO QUANTEL MEDICAL.

DICOM IMAGING



A world premiere in ophthalmic ultrasound: new Full HD screen with greyscale display compliant with section 14 of the DICOM standard.

- Constant and standardised image quality.
- Reliable image interpretation.



ABSolu 8 FUNCTION WIRELESS FOOTSWITCH



- Adjustable Gain (+ and -).
- Freeze/unfreeze image.
- Viewing of Cineloop images (forward and reverse function).
- Images saved in the patient's file.
- Tag on the Cineloop.






■ NEW UBM IMAGING

UBM technology makes it possible to **diagnose the structures behind the iris**, that other technologies cannot visualize. Quantel Medical now offers **optimised UBM technology**:

- **new signal processing for enhanced resolution and penetration,**
- **linear transducer motion to optimise image quality,**
- electromagnetic technology to increase speed acquisition and comfort of use,
- **Clearscan™** compatible: rapid and comfortable examination.

■ GLAUCOMA MODULE

All the **semi-automatic quantification tools** are available on ABSolu (AOD, TIA, IT, ARA, LV) and **facilitate examination and understand the mechanisms of the iris, the lens and ciliary bodies** in patients with glaucoma.

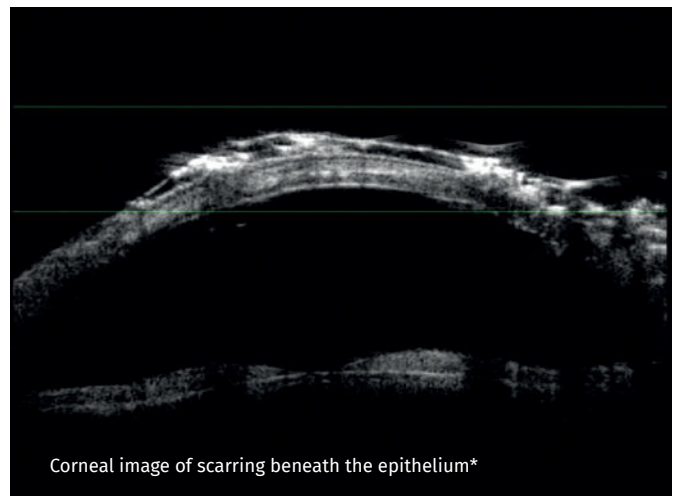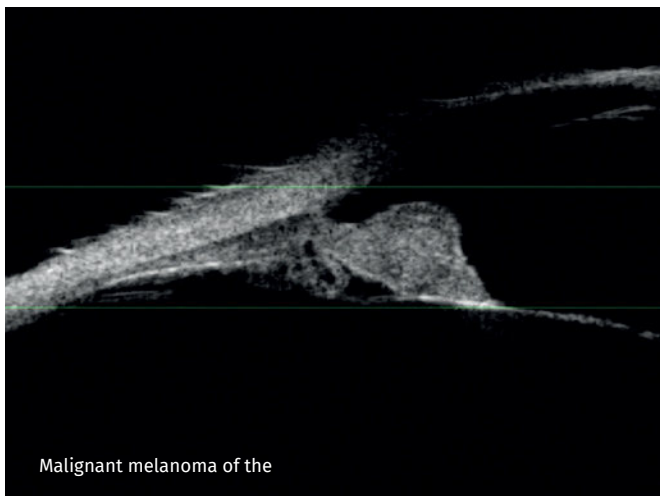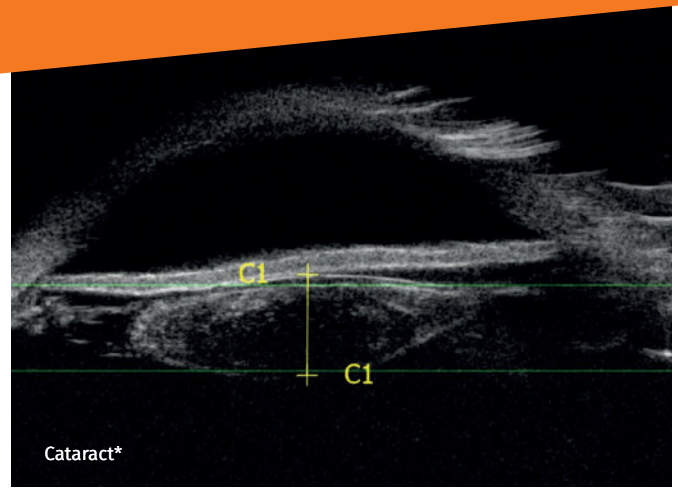

* Peter Good, MD, Birmingham and Midland Eye Center (Birmingham, UK).

■ STANDARDISED ULTRASOUND

With **numerous enhancements** that make it **easier and more intuitive to use**, ABSolu remains the only ultrasound platform that meets **Professor Karl Ossoinig's criteria**.

The **S mode** allows for:

- diagnosis of tumour lesions,
- diagnosis of retinal/vitreous membrane detachment,
- diagnosis of Graves' disease.

■ A-SCAN BIOMETRY AND B MODE BIOMETRY

The A-scan biometry and B mode biometry modules **facilitate measurement of the axial length** in eyes of **all types**:

- moderate to dense cataract,
- long eyes or posterior staphylomae.

This measurement is **facilitated by the ProBeam™ probe** (biometric probe with on-board laser) which makes for better cooperation from the patient during examination.

TECHNICAL SPECIFICATIONS



B SCAN MODES

Grey levels:	256
Adjustable gain:	20 to 110 dB
Adjustable Time Gain Control (TGC):	0 to 30 dB
Adjustable dynamic range:	adjustment from 25 to 90 dB (for 15 and 50 MHz - 80 dB for 20 MHz 5A)
Image post-processing tools:	filters (algorithm and colors), calipers, areas, angles, markers, comments
Glaucoma quantifying semi-automated tools:	AOD 500 & 750, TIA, IT 750 & 2000, ARA 500 & 750, TISA 500 & 750, LV up to 400 images
Cineloop in B mode:	up to 400 images

POSTERIOR POLE EXAMINATION

Magnetic 15 MHz probe

Transducer frequency:	15 MHz
Angle of exploration:	50°
Depth of exploration:	60 mm (2.36")
Focus:	24 mm (0.94")
Depth of field:	12 mm (0.47")
Axial resolution:	115 µm
Lateral resolution:	400 µm
Frame rate acquisition:	up to 16 Hz
Accelerometer for probe localization	

Magnetic Annular 5 rings 20 MHz probe

Transducer frequency:	20 MHz – Annular 5 rings
Angle of exploration:	50°
Depth of exploration:	60 mm (2.36")
Focus:	22 mm (0.87")
Depth of field:	20 mm (0.79")
Axial resolution:	80 µm
Lateral resolution:	200 µm
Frame rate acquisition:	up to 16 Hz
Accelerometer for probe localization	

UBM & ANTERIOR SEGMENT EXAMINATION

Magnetic 50 MHz UBM probe with linear scanning

Transducer frequency:	50 MHz
Linear transducer movement:	16 mm (0.63")
Focus:	10 mm (0.39")
Axial resolution:	35 µm
Lateral resolution:	60 µm
Accelerometer for probe localization	

STANDARDIZED A MODE

Digitally programmed S-shaped amplifier characteristics and comprehensive design criteria for standardized echography and tissue differentiation according to Karl C. Ossoinig MD. Automatic tissue sensitivity determination with specific gain value recorded.

Diagnosis functions featuring: Lesion Q1, Retina A1, Retina Q2, muscular profile with Optic nerve measurements

Probe Frequency:	8 MHz parallel beam
Cineloop in A mode:	up to 400 images
Depth:	orbit 80 µs, eye 40 µs, zoom 20 µs
Distance measurement between 2 gates with adjustable velocity	

BIOMETRY

Adjustable gain:	20 to 110 dB
Adjustable Time Gain Control (TGC):	0 to 30 dB
11 MHz Probe	
Transducer frequency:	11 MHz
Tip diameter:	7 mm (0.28")
Electronic resolution:	0.04 mm (0.0016")
Depth of exploration:	40/80 mm (1.57"/2.36") on 2048 points
Aiming beam:	LED or laser beam ProBeam™
Contact and immersion techniques compatible	

Axial length measurements

Ultrasound propagation velocity adjustable per segment (anterior chamber, lens, vitreous) and IOL and vitreous material

Built-in pattern recognition:	Phakic, Dense/Long, Aphakic, PMMA, Acrylic and silicon for pseudo-phakic eyes
Acquisition modes:	Automatic, Auto+save, manual Automatic detection of scleral spike

Automatic calculation of standard deviation and average total length (series of 10 measurements)

IOL calculation

SRK-T, SRK 2, HOLLADAY, BINKHORST-II, HOFFER-Q, HAIGIS

Post-op refractive calculation:

- Pre-op and Post-op refraction, Pre-op and Post-op keratometry
- 6 different methods for keratometric correction and implant calculation:
History derived, refraction derived, contact lens method, Rosa regression, Shammass regression, Double K/SRK-T (Dr. Aramberri's formula)
9 values bracketed for desired ametropia for each IOL (IOL increment steps: 0.25D or 0.50D)
Simultaneous display of 4 different IOL calculations

DATA MANAGEMENT

Built-in physician and patient database
Exportation of still images and video sequences
Customizable digital and printed reports
DICOM* and/or EMR compatible
Compatible with PC, USB video and DICOM printers
Storage capacity: no restriction of number of exams per patient *in options

GENERAL INFORMATION

Connection 5 USB ports (1 on the base – 4 on the bottom of the screen)
HDMI and Ethernet outlets
Windows 10 embedded exploitation system
HDD 1TB - SSD128 Gb – RAM 16 Gb
No restriction of storage in patient file

Electrical requirements

Power supply:	80-264 Vac
Frequency:	47/63 Hz
Power:	60 VA max

Features

Overall dimensions:	Height 445 mm (17.51") - Depth 285 mm (11.22") - Width 545 mm (21.46") (W/O probe holders) and 840 mm (33.07") with all probes
Screen dimensions:	21" inch HD (1920*1080p)
Weight:	10.6 kg (23.37 lbs) (w/o probes)

Specifications are subject to change without notice.

©2019. Quantel Medical, ABSolu is a registered trademark of Quantel Medical. All rights reserved.

www.quantel-medical.com

Headquarters

Quantel Medical
11, rue du Bois Joli - CS40015
63808 Cournon d'Auvergne – FRANCE
Tel: +33 (0)4 73 745 745
Email: contact@quantel-medical.fr

North America

Quantel Medical USA
2313 Ridge Road Suite 105A
Rockwall, TX 75087 – USA
Tel: +1 888 660 6726
Email: info@quantelmedical.com

Poland

Quantel Medical
ul. Raclawicka 93
02-634 Warszawa - POLAND
Tel: +48 22 5210111
Email: info@quantel-medical.pl



Quantel
medical



BY LUMIBIRD

ISO 9001 : 2015 – ISO 13485 : 2016

Representative Offices

Thailand, Chiang Mai
Brazil, Rio De Janeiro